

Bioengineering 208

Magnetic Resonance Imaging


Winter 2007

Lecture 5

- MRI Artifacts
 - Noise spikes
 - Clipping
 - Gibbs Ringing
 - Quadrature ghost
 - Wraparound
 - Motion
 - Chemical Shift
- SNR in MRI
 - RF Coil
 - Magnetization
 - Sampling time

E. Wong, BE208, UCSD Winter 2007

Normal Image

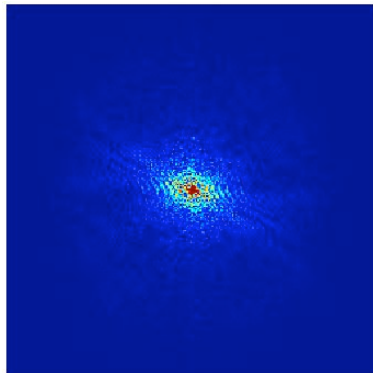

K-space


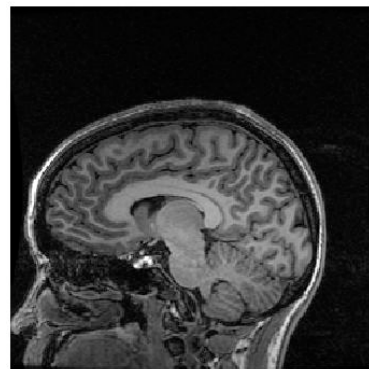


Image space

E. Wong, BE208, UCSD Winter 2007

Noise Spike

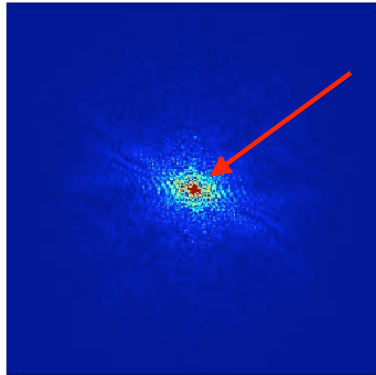

K-space


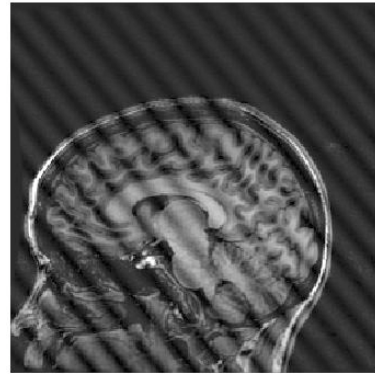


Image space

- Localized in K-space
- Extends outside object in image space
- Come from arcing, loose connections, ground spikes

E. Wong, BE208, UCSD Winter 2007

More Noise Spikes

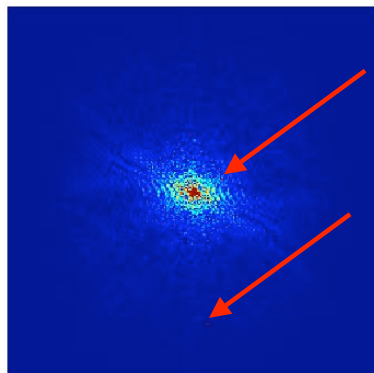

K-space


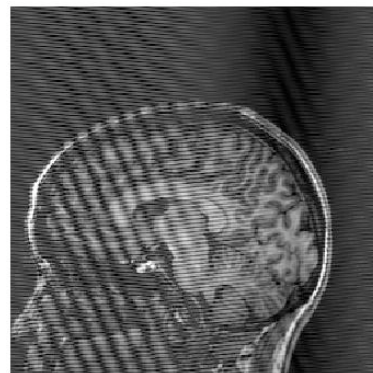


Image space

- Multiple spikes create multiple sinusoids and generate 'herringbone' patterns

E. Wong, BE208, UCSD Winter 2007

Data clipping

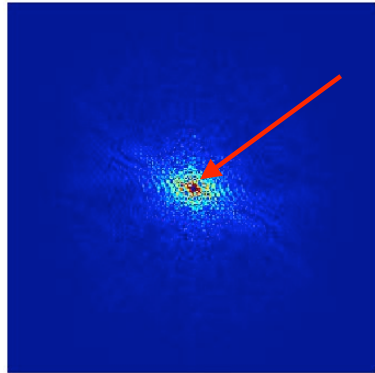

K-space


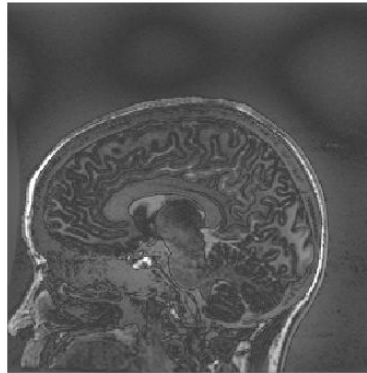


Image space

- Center of K-space over-ranges ADC and clips
- Image is (correct image) - (low frequency image)

E. Wong, BE208, UCSD Winter 2007

Data clipping

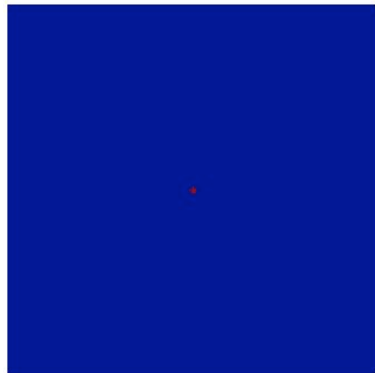

K-space


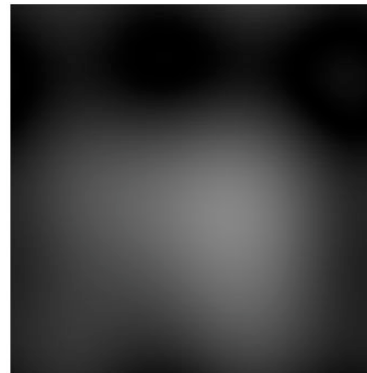


Image space

- Here is the data that was clipped

E. Wong, BE208, UCSD Winter 2007

Gibbs Ringing

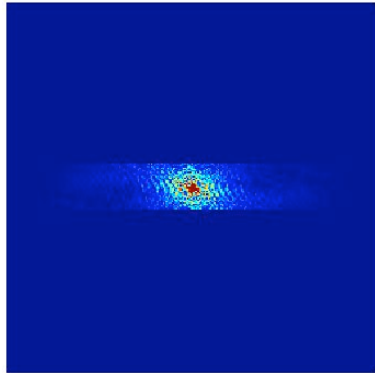

K-space


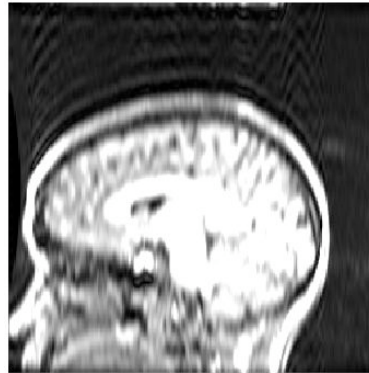


Image space

- Data is truncated before it decays into the noise
- Result is an image convolved with FT of the window in k-space

E. Wong, BE208, UCSD Winter 2007

Quadrature Ghost

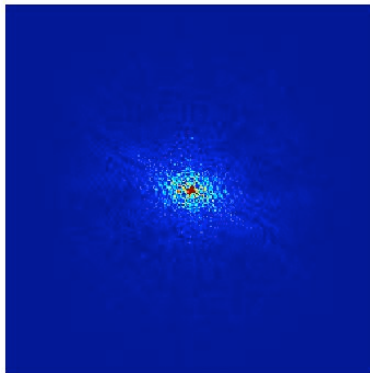

K-space


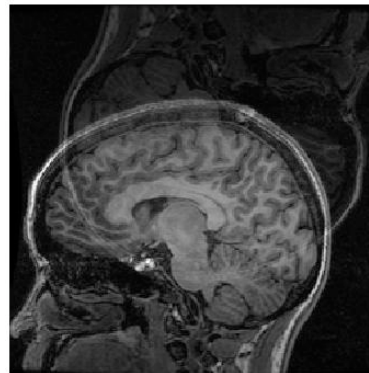


Image space

- K-space data is a superposition of good_data and good_data^*
- \Rightarrow Image space is a superposition of $\text{good_image}(x,y)$ and $\text{good_image}(-x,-y)$

E. Wong, BE208, UCSD Winter 2007


Wraparound

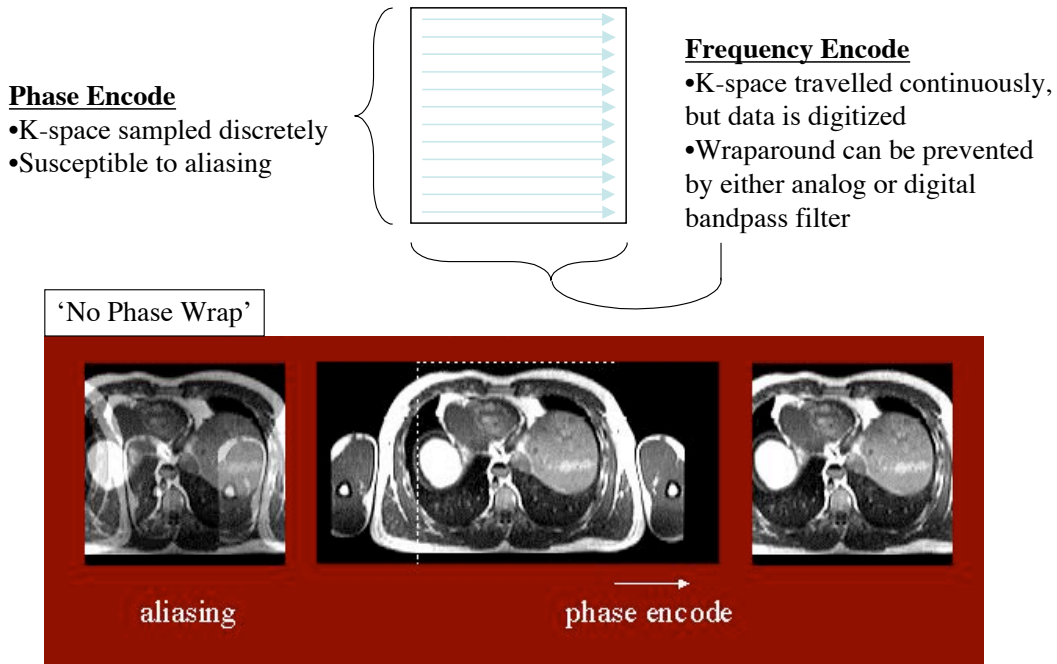


E. Wong, BE208, UCSD Winter 2007

<http://www.fmrib.ox.ac.uk/~peterj/lectures/kpace/img034.GIF>

Motion Artifact

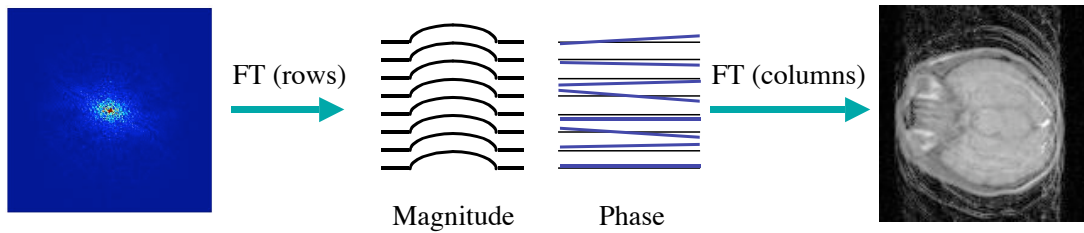

- Motion between TR periods generates inconsistency between lines of K-space
- Ghosts propagate in the phase encode direction
- Period motion generates structured ghosts (analogous to EPI Nyquist Ghosts)

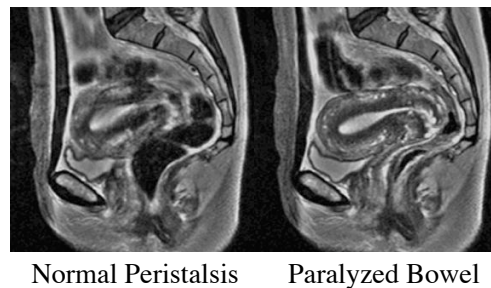


E. Wong, BE208, UCSD Winter 2007

<http://www.rad.pulmonary.ubc.ca>

Chemical Shift


- Magnetic field of electron clouds shields nucleus from external magnetic field
- =>Actual magnetic field experienced by nucleus is smaller than applied field
- Differences in local field are called chemical shift, and are measured in PPM
- Water and fat differ in chemical shift by 3.5 PPM = 440Hz at 3T
- Chemical shift causes phase twist across readout
- Fourier shift theorem tells you how far things are shifted

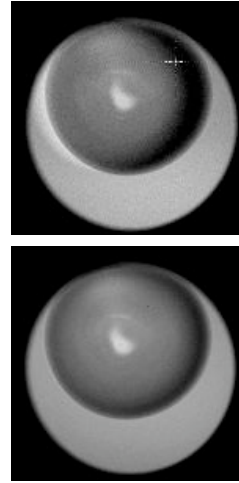

http://chickscope.beckman.uiuc.edu/roosts/carl/artifact/cs_a001.gif


E. Wong, BE208, UCSD Winter 2007

CONVENTIONAL IMAGING

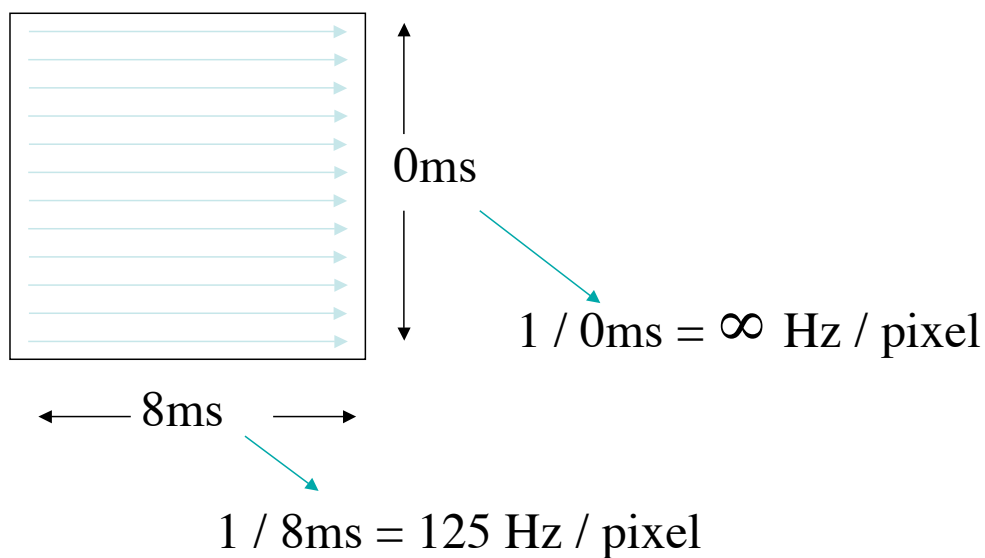

E. Wong, BE208, UCSD Winter 2007


Off Resonance Behavior : EPI

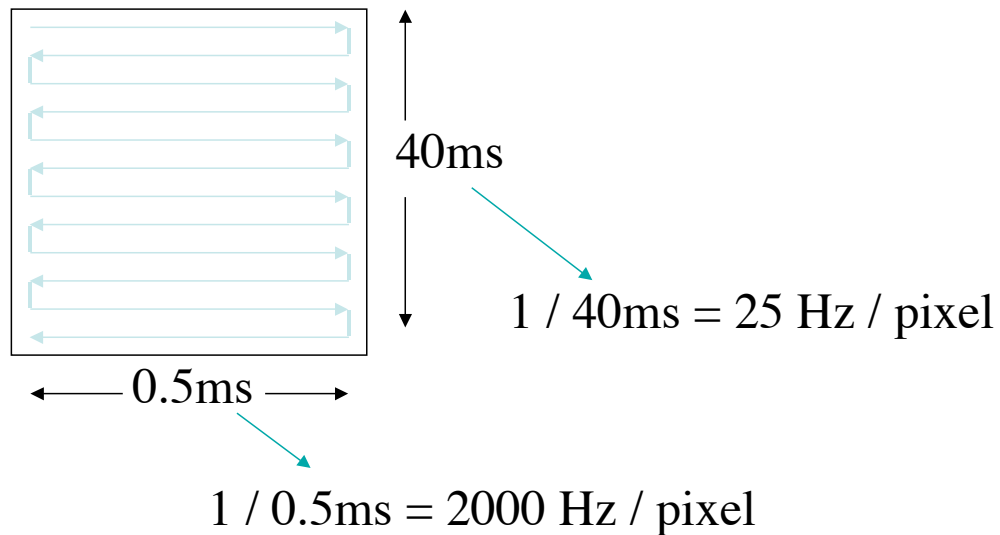

E. Wong, BE208, UCSD Winter 2007

Signal to Noise Ratio in MRI

$$SNR \propto (\text{coil_factor}) \times (\text{magnetization_factor}) \times (\text{sampling_factor})$$

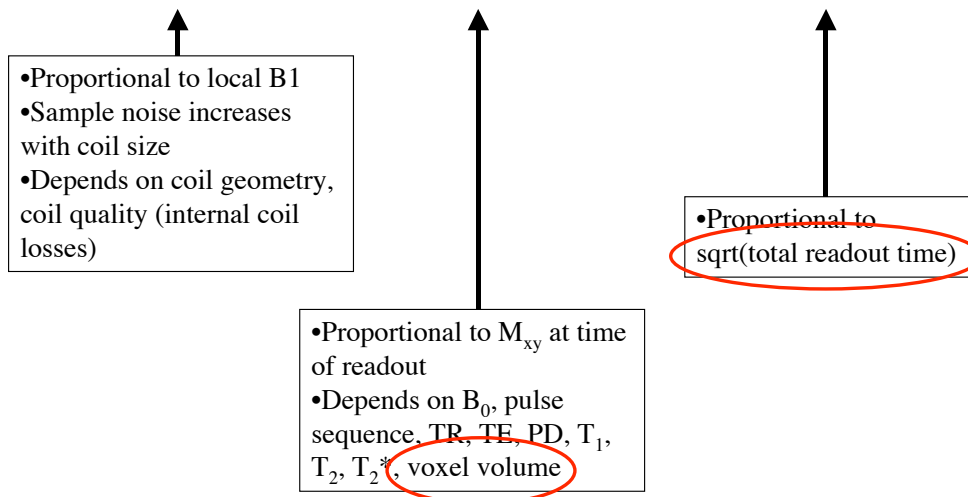

$$SNR \propto (\text{voxel_volume}) \sqrt{\text{total_readout_time}}$$

E. Wong, BE208, UCSD Winter 2007